


# Qualitative Analysis Report

<b>Data Filename</b>	Ziegler0398.D	<b>Sample Name</b>	TZ110A-1
<b>Sample Type</b>		<b>Position</b>	42
<b>Instrument Name</b>	GCMS5977B	<b>User Name</b>	NG
<b>Acq Method</b>	S1016_8a.M	<b>Acquired Time</b>	4/15/2021 12:39:07 PM (UTC+02:00)
<b>IRM Calibration Status</b>	Not Applicable	<b>DA Method</b>	TheSysNG.m
<b>Comment</b>	S1016_8a.M		

<b>Expected Barcode</b>	<b>Sample Amount</b>
<b>Dual Inj Vol</b> 0.5	<b>TuneName</b> etune.u
<b>TunePath</b> D:\MassHunter\GCMS\1\5977	<b>TuneDateStamp</b> 2021-03-19T10:46:20+01:00
<b>MSFirmwareVersion</b> 6.00.34	<b>OperatorName</b> NG
<b>RunCompletedFlag</b> True	<b>Acquisition Time (Local)</b> 4/15/2021 12:39:07 PM (UTC+02:00)
<b>Acquisition SW Version</b> MassHunter GC/MS Acquisition 10.0.368 14-Feb-2019 Copyright © 1989-2018 Agilent Technologies, Inc.	<b>SingleQuadrupole Driver Version</b> 10.0.0.0
<b>SingleQuadrupole Firmware Version</b> 6.00.34	

## Chromatograms

Fragmentor Voltage      Collision Energy 0      Ionization Mode EI

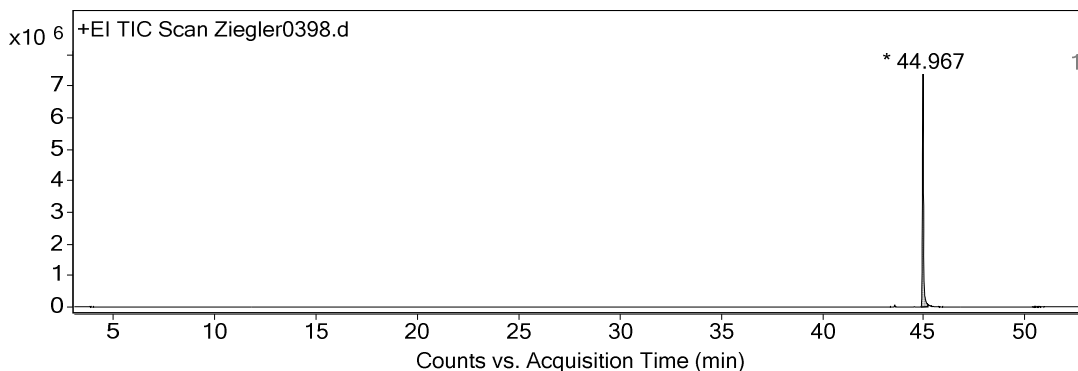


## Integration Peak List

Peak	Start	RT	End	Height	Area	AreaSumPercent
1	44.865	44.967	45.207	7369201.17	26876031.71	100

## Spectra

Collision Energy 0      Ionization Mode EI

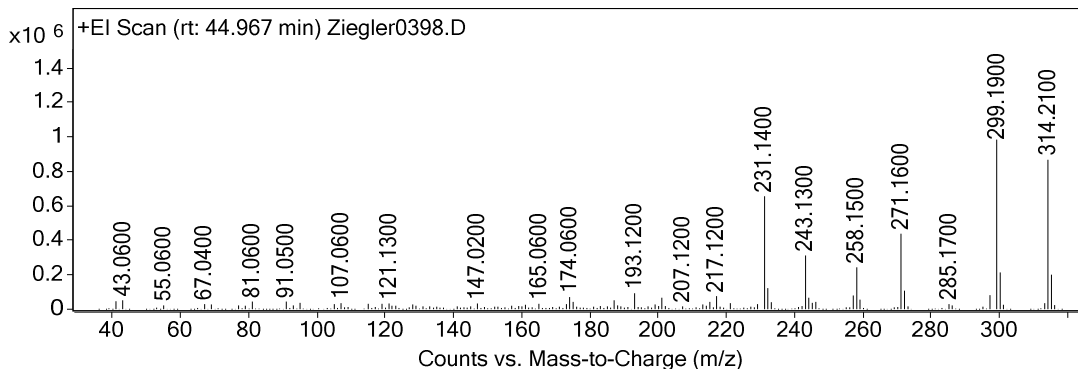

--- End Of Report ---